



BRUKER

Changing Microbiology

IR Biotyper[®]

Microbial strain typing for real-time epidemiology

Innovation with Integrity

GP

IR Biotyper

Supporting proactive infection control

Efficient microorganism strain typing is vital in healthcare settings, for infection control, epidemiological studies, and to better understand the causes of infection. However, traditional strain typing technologies like pulsed-field gel electrophoresis (PFGE), multi-locus sequence typing (MLST) and whole-genome sequencing (WGS) are time-consuming and resource-intensive, and not commonly available in microbiological laboratories.

Fast, easy-to-use, and economical, the IR Biotyper addresses this challenge by using infrared spectroscopy to classify microorganism strains with high specificity. Its discriminatory power is comparable to routine molecular genetic methods.

The IR Biotyper's ability to perform real-time strain typing, along with its efficient software, allows for proactive infection control.



Benefits of using the IR Biotyper

Implementing the IR Biotyper in your hospital hygiene management system will:


- Enable swift identification of microbial outbreaks
- Allow investigation of unusual patterns in a set of samples
- Enable classification of isolates based on predefined classification models, e.g., allowing fast detection of known serotypes and strains
- Allow transmission routes to be monitored in real time
- Support preventive action through routine screening
- Enable improved data-based hygiene management through further analytical studies; however, the IR Biotyper is not intended for patient management



The principle of FT-IR

The IR Biotyper uses Fourier Transform Infrared (FT-IR) spectroscopy to analyze the molecular vibrations caused by absorption of infrared light. Different chemical structures vibrate at different wavenumber regions – for example, the carboxyl group in fatty acids (and lipids) vibrates at 2800–3000 cm^{-1} , the amide group in proteins vibrates at 1500–1800 cm^{-1} , and the carboxy group in polysaccharides vibrates at 900–1200 cm^{-1} .

The IR Biotyper offers the option to use data from all these regions, to provide information about the full range of diagnostic molecules present in the sample. In routine use, the polysaccharide region (900–1200 cm^{-1}) is the most useful one, as this part of the spectrum is like a 'fingerprint', providing information about the carbohydrates present in many molecules such as glycoproteins, and allowing microorganisms such as *Streptococcus pneumoniae* serotypes to be classified.

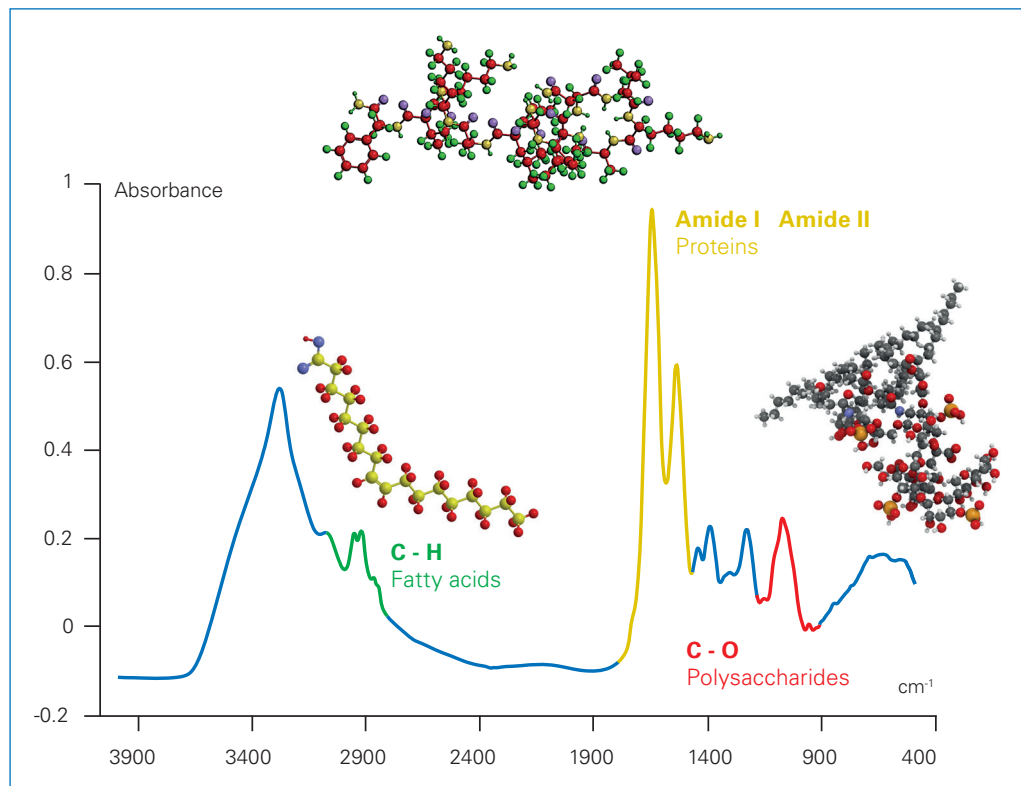


By default, the IR Biotyper analyzes IR spectra in the wavenumber range typical for carbohydrates (red), but other regions such as those indicating fatty acids (green) and proteins (yellow) can easily be selected for analysis in the software as well.

Simple workflows for rapid processing

The IR Biotyper is quick and easy to use. Following harvesting, preparation of a suspension, spotting on a 96-well silicon microtiter sample plate and drying, the plate is simply inserted into the instrument, and analysis begins.

The instrument processes an individual spot in about a minute, meaning that an entire plate can be analyzed in about 90 minutes. Across the whole workflow, and using three replicates per isolate, this means that up to 30 isolates can be analyzed in 3 hours.

96-Spot silicon microtiter plate and IR Biotyper Kit

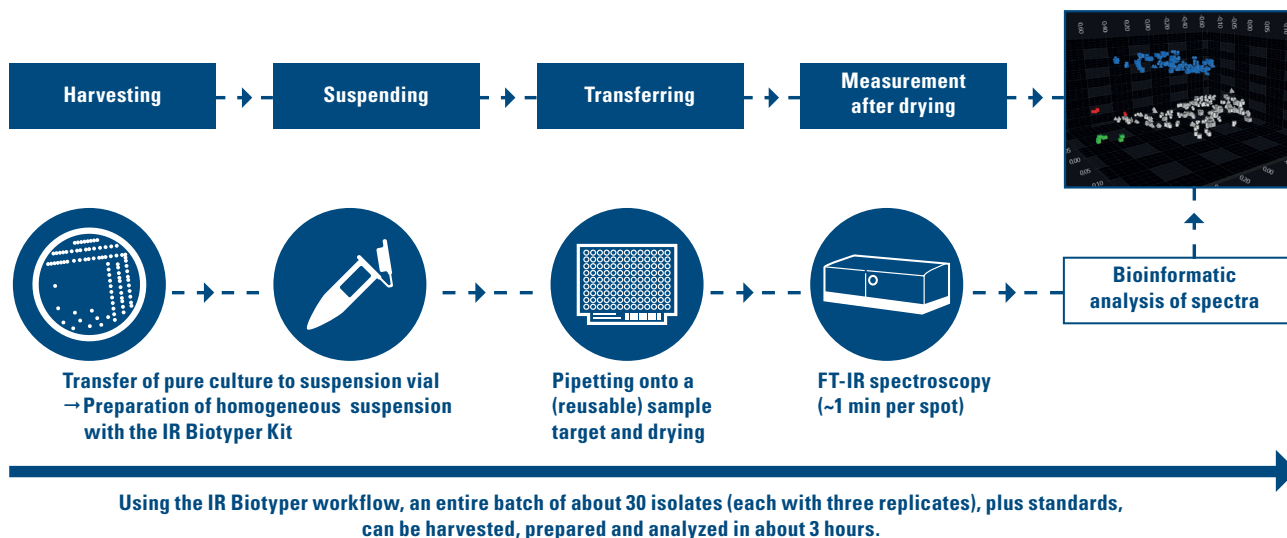

Integrated workflows for microorganism identification and strain typing

The IR Biotyper and Bruker's MALDI Biotyper® can now be combined into a single seamless workflow. Data from the MALDI Biotyper – which uses MALDI-TOF MS to identify microorganisms to species or genus level within a few minutes – can be imported into the IR Biotyper software, and once analyzed, the entire set of results can be exported to the laboratory's LIMS in CSV format.

Intuitive software aiding epidemiology


Clear data visualization through reliable and intuitive data analysis

Strain typing results achieved with FT-IR spectroscopy are equivalent to molecular methods, and this has been demonstrated by strain typing of over 240 clinical isolates of vancomycin-resistant *Enterococcus* (VRE) using genomic sequencing and the IR Biotyper (see dendrogram on the following page).

In addition, data obtained using the IR Biotyper are easy to interpret, with smart isolate classification complemented by convenient visualization tools.

Real-time isolate quality-checking and classification

Isolate classification using the IR Biotyper software is based on an artificial neural networks and/or a Support Vector Machine algorithm. Classifications can be based on predefined or customized models, allowing fast identification of serotypes, serogroups or strains previously identified e.g., during an outbreak, and supporting fast preventive action. Classifications rely on a score value, which is rendered in real-time using a 'traffic light' system for at-a-glance understanding and streamlined workflows.

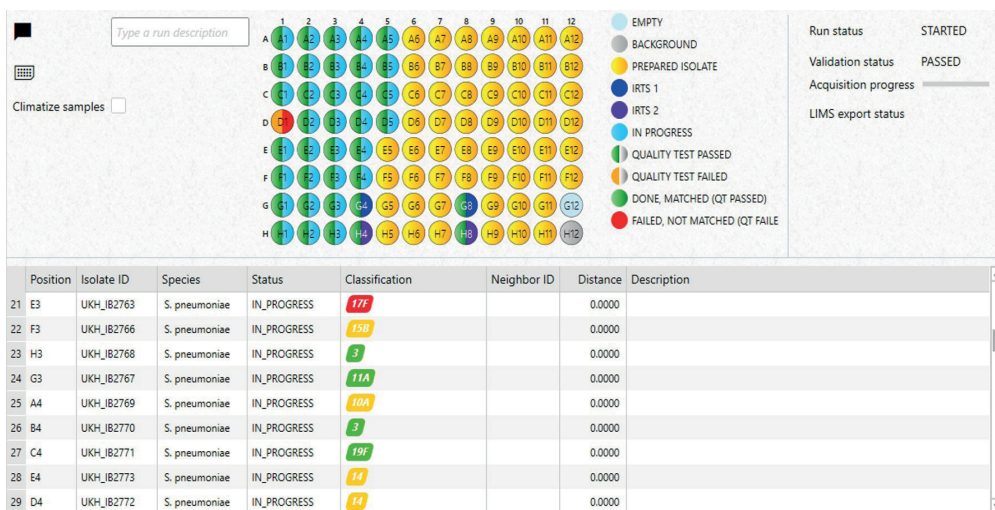

Fast and automated classification of pneumococci serotypes



Up-to-date software for streamlined operation

- Customizable isolate metadata, including biological, such as multi-locus sequence typing (MLST), pulsed-field gel electrophoresis (PFGE), virulence factors and resistances; and circumstantial, such as location, isolation date, and matrix
- Data can be imported from MALDI Biotyper into the IR Biotyper software, plus laboratory information management system (LIMS) export
- Simple building and automated application of classifiers based on artificial neural networks (ANN) and Support Vector Machine (SVM) for isolate classification
- Built-in classifiers, subject to regular updates
- 3D principal component analysis (PCA) plots and one simple color coded (traffic light) report
- Straightforward reports for classification results


Versatile data exploration options

Results can be displayed in table format, or visualized graphically using distance matrices, dendrograms or scatter plots.

Isolate clustering can be assessed using distance matrix plots or dendrograms, as shown in this dendrogram example of *Klebsiella pneumoniae* isolates for outbreak analysis.

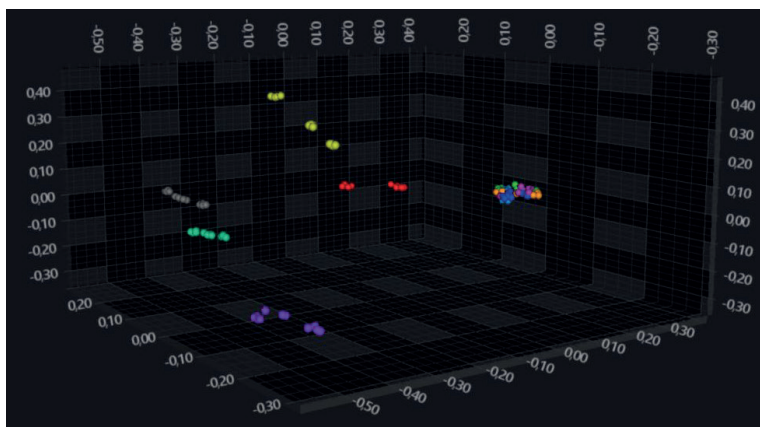

Results of principal components analysis can be visualized using 2D or 3D scatter plots, as shown here for *Klebsiella pneumoniae* isolates.

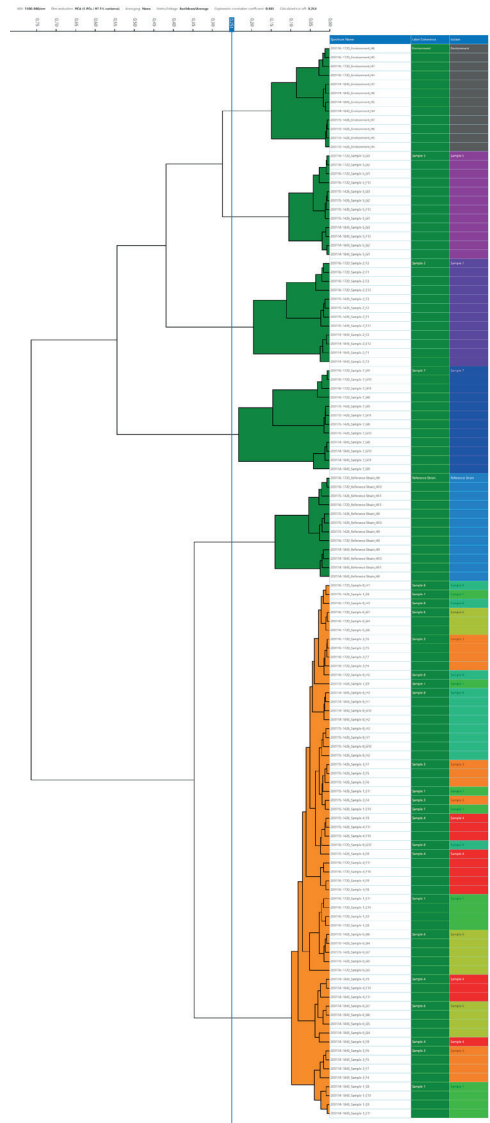




Dr. Juan de Dios Caballero

Associate Dr. in Hospital Ramón y Cajal, Madrid

"We have successfully tested the IR Biotyper for the identification of outbreaks caused by ceftazidime/avibactam-resistant *Klebsiella pneumoniae*, GES-carbapenemase-producing *Pseudomonas aeruginosa*, and linezolid-resistant *Enterococcus faecium*. In all cases we have observed good correspondence with classical typing techniques (PFGE) and/or with massive sequencing techniques.

We are also exploring the IR Biotyper to distinguish contaminating microorganisms from blood cultures and joint prosthesis infections. In both cases we are isolating coagulase-negative staphylococci from diverse samples and are quickly testing if we have the same microorganism."



Dr. Cristina Pitart

ID and AST Specialist in Microbiology Dept. Hospital Clínic de Barcelona


"We are currently using the IR Biotyper for the early detection of outbreaks. Diverse clinical and surveillance samples of all vancomycin-resistant *Enterococcus faecium*, carbapenemase-producing *Enterobacterales*, and multidrug-resistant *Pseudomonas aeruginosa* strains are measured by the IR Biotyper and archived. When an accumulation of cases occurs, the clonality of the strains is analyzed by the IR Biotyper. We have very good experience with *K. pneumoniae*, *P. aeruginosa* and *Enterobacter cloacae*. Thus, thanks to the speed and good discriminative power of the method, we can corroborate the nosocomial transmission of these microorganisms and establish more rapid and effective prevention measures. "



Dr. Elena De Carolis

Department of Microbiology at the University Hospital Fondazione Policlinico A. Gemelli, Rome

"The IR Biotyper is going to become a reliable and useful tool to perform a "Real-Time" hospital surveillance strategy in our hospital. Thanks to the biochemical fingerprint approach based on FT-IR spectroscopy, it is possible to type diverse bacterial isolates using a rapid and easy to use technology. Showing good correlation with molecular typing technologies, the IR Biotyper will help to overcome the spread of multidrug resistant microorganisms in the future."



Order information

IR Biotyper

Part No. 1845471

High-performance FT-IR spectrometer with capability for analyzing 96-spot silicon microtiter sample plates, and updated software for sample setup and data analysis.

96-Spot silicon microtiter plates

Part No. I23258P

Set of five reusable plates with 96 positions each designed for use with the IR Biotyper.

IR Biotyper Kit

Part No. 1851760

Includes two bacterial IR test standards (IRTS 1 and IRTS 2) for five runs, and sample preparation vials for 50 isolates.

Not for use in clinical diagnostic procedures.
Please contact your local representative for availability in your country.

IR Biotyper® and MALDI Biotyper® are registered trademarks of the Bruker group of companies.

Online information
bruker.com/microbiology

 **Bruker Daltonics GmbH and Co. KG**

Bremen · Germany
Phone +49 (0) 421-2205-0

info.md@bruker.com

Bruker Scientific LLC

Billerica, MA · USA
Phone +1 (978) 663-3660

